


**Certificate of Analysis
 Technical Data for Validation
 Total Chlorine Powder Pillows
 (0.02 – 2.00 mg/L)**

The data for this Certificate of Analysis follows the procedures in USEPA Approved Hach Method 8167 and ISO 8466.

Catalog Number	2105669
Date of Certificate	August 19, 2015
Number of Lots	50

Sensitivity (0.010 Abs Change)	0.02 mg/L Cl ₂
Reagent Blank	0.01 mg/L
Accuracy	1.5 %
Confidence Interval (95%)	0.3 %
Method Standard Deviation	0.03 mg/L Cl ₂
Method Variation Coefficient	1.5 %
Detection Limit	0.02 mg/L Cl ₂
Quantitation Limit	0.05 mg/L Cl ₂

Expected Value mg/L Cl ₂	Obtained Value mg/L Cl ₂
2.00	1.97

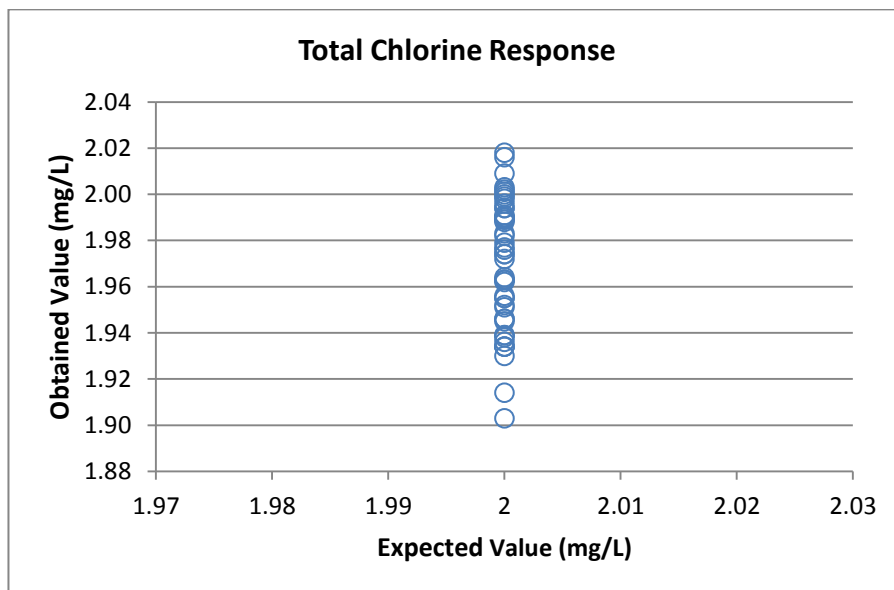

Scott Als, Quality Control Chemist

Scott Als

